



Figure 1.  
the electrode leads

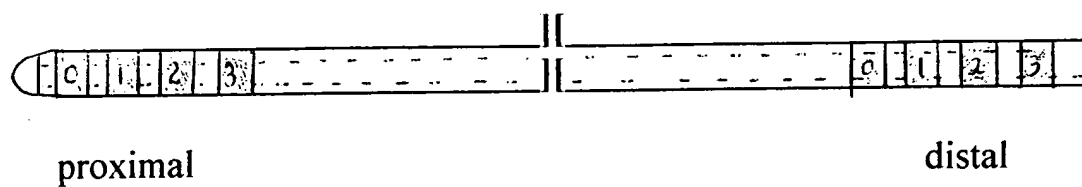

O.D. ~ 2 mm.


Figure 2.  
neurovascular supply of the phallus  
corpus cavernosum

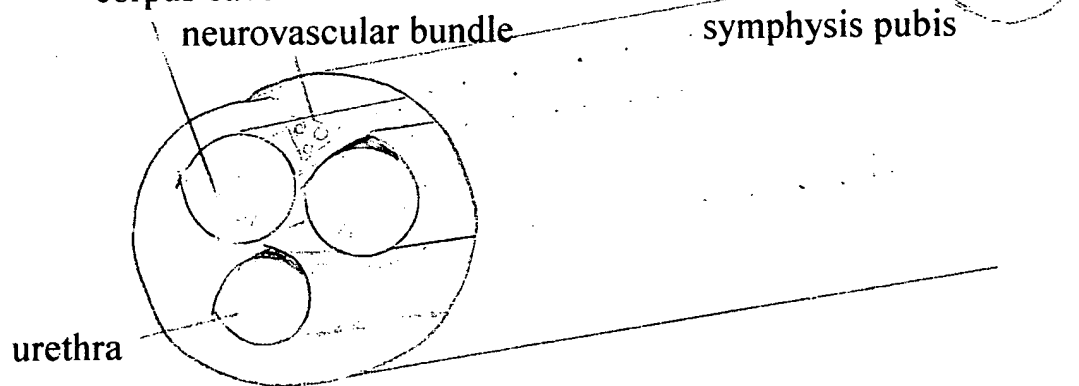

10005390-120301

Figure 3.

the test stimulation;  
phallic, percutaneous

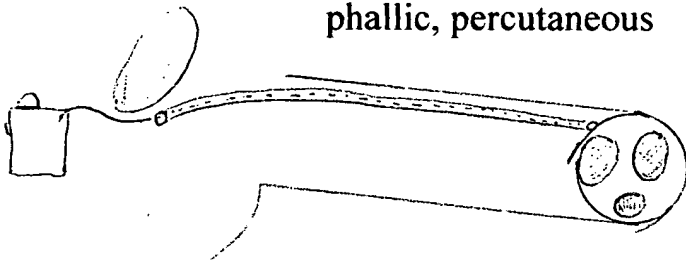

circumferential, transcutaneous


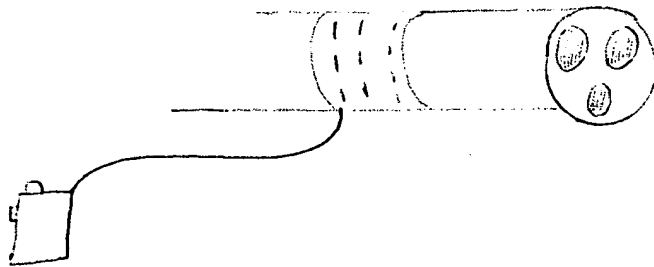


Figure 4.

inventive device in surgical position

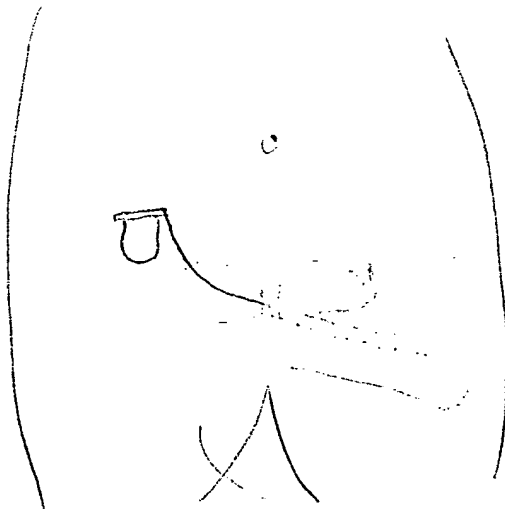

10005350-120304